


DATA SHEET

# Vault Access System

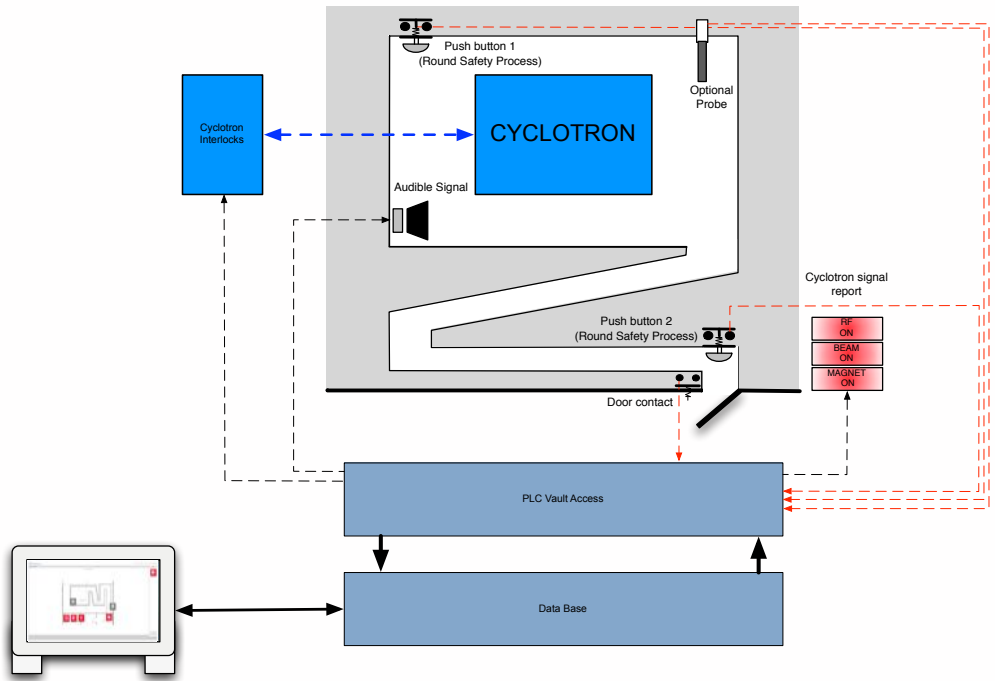

### Vault Access System :

V.A.S. manages the process of access authorization to the cyclotron room (vault).

It authorizes cyclotron start-up only after ensuring that no one remains in the vault.

Following this authorization, it also informs on cyclotron status (Magnet, RF and Beam).

V.A.S can also manage vault access authorization after a beam, depending on the residual radioactivity level (optional)

### Operating Process

V.A.S controls vault access safely.

V.A.S allows vault access by:

- > Authorizing cyclotron beam
- > Managing Round process
- > Monitoring vault door contacts
- > Informing staff on cyclotron status
- > Measuring vault residual radioactivity level before authorizing vault access (optional).

Database collects the information for displaying, alerting and backup.

The displayed module's screens are specifics but can be designed according to your needs.

Database can be used in maintenance mode or multi-site mode through remote access



Acist Healthcare solution. is designed to collect the facility information.

Acist Healthcare solution. allows supervising, alerting and acting on installation in order to preserve property and persons.

Acist Healthcare solution. is equipped with different modules to control radiation, to manage transfer or the cyclotron access. These modules are integrated in function of your needs.

**Acist Healthcare solution**

[www.psi-nm.com](http://www.psi-nm.com)

## V.A.S. Characteristics

Round System	
Push Button	Normally Open - DC 24V
Audible	90 db
Timer	set by Customer
Door Status	define by 1 serial wirred sensors.
Signal	Electrical Signal
Type	Cyclotron Beam ON
Information	Cyclotron RF ON Cyclotron MAGNET ON
Power	Electrical (DC 24V)
Cyclotron interlocks	
Hard Wire Chain	Vault Safety Condition

## Standart Package

Cyclotron Signal Report	3 (Beam On, RF On, Magnet On)
Buzzer	1
Door Contact	2
Round Buttom	2

## Available Options

Additional Remote Signal

GM Probe in Vault

*One probe can be used to measure activity inside the vault after a cyclotron beam. In this case, the authorization of access in cylotron vault is given by the probe. This option is included if the RPS module is installed.*

Extended Warranty (up to 5 years)

- **VAS is a Vault Access System**
- **VAS displays Vault Access and Cyclotron status**
- **VAS manages alarm and history**
- **VAS manages user rights**
- **VAS manages the vault access request after a cyclotron beam**
- **VAS supports remote access**
- **VAS is part of Acist Healthcare solution**

## PSI Nuclear Medicine

23 Rue des Loges  
91410 St Cyr sous Dourdan - FRANCE

Phone : +33 (0) 632 661 514

Fax : +33 (0) 466 774 510

Mail : [contact@psi-nm.com](mailto:contact@psi-nm.com)

[www.psi-nm.com](http://www.psi-nm.com)